

Mouse Osteopontin N-Half Assay Kit - IBL

96 Well

Please read carefully this instruction prior you use this assay kit.

INSTRUCTIONS FOR USE

This product is for research use only and is not intended for diagnostic use.

KIT COMPONENT

1	Precoated plate: (Anti-OPN N-Half (34E3) Mouse IgG MoAb A.P.)	96Well x 1
2	Labeled antibody conc.: (30X) HRP conjugated Anti-Mouse OPN (O-17) Rabbit IgG Fab' A.P.)	0.4mL x 1
3	Standard: (Recombinant Mouse OPN N-Half)	0.5mL x 2
4	EIA buffer	30mL x 1
5	Solution for labeled antibody	12mL x 1
6	Chromogen: TMB solution	15mL x 1
7	Stop solution	12mL x 1
8	Wash buffer conc.	50mL x 1

MEASURING SAMPLES

Mouse EDTA-Plasma, Urine and Cell culture supernatant

Please store all samples at -80°C before use because OPN molecule is unstable protein. Since measured value falls by being left in room temperature or repetition of freeze/thaw cycles, cautions are required. In many cases of normal mice, it is recognized that OPN N-Half is present in minute amounts in their plasma. Therefore, the concentration of OPN N-Half in mouse plasma is expected to be below the detection sensitivity of this kit. The assay by serum samples give any values, but it might be not reflected correct values, because OPN is unstable and is easily cleaved by thrombin. Since it is easy to decompose a urine sample, we recommend to add PMSF (protease inhibitor) etc. Moreover, when it cannot measure immediately after extraction, please store at -80°C or less. The recommended dilution for cell culture media samples is various by using cells, therefore, the dilution rate should be optimized by each laboratories. Both recombinant and native forms of Mouse OPN N-Half can be detected with the kit.

PRINCIPLE

This kit is a solid phase sandwich ELISA (Enzyme-linked Immunosorbent Assay). As a primary antibody is coated on a plate, samples and standard are added into the wells for 1st reaction. After the reaction, HRP-conjugated secondary antibody is added into the wells for 2nd reaction. After washing away unbound the secondary antibody, Tetra Methyl Benzidine (TMB) is added to the wells and color develops.

OPERATING PRECATION

- Test samples should be measured soon after collection. For storage of samples, store them frozen and do not repeat freeze/thaw cycles. Thaw the test samples at a low temperature and mix them completely before measurement.
- Test samples should be diluted with "4, EIA buffer" contained in this kit.
- Duplicate measurement of test samples and standards is recommended.
- Standard curve should run for each assay.
- Use test samples in neutral pH range. The contaminations of organic solvent may affect the measurement.
- All reagents should be brought to room temperature (R.T.) and mixed completely and gently before use. After mixing them, make sure of no change in quality of the reagents.
- Use only "8, Wash buffer conc." contained in this kit for washing the precoated plate. Insufficient washing may lead to the failure in measurement.
- Fill the wash buffer each well, invert the plate and make sure the liquid is completely removed by shaking it off if you use a washing bottle. Repeat this washing process several times as instructed in order to avoid any insufficient washing process.
- After remove the wash buffer, tapping the plate against a clean paper towel for completely removing the liquid from the wells and make sure the paper towel is not contact with inside of the wells in this process.
- "6, Chromogen - TMB solution" should be stored in the dark due to its sensitivity against light. It should be also avoided contact with metals. Required quantity should be prepared into a collecting container for each use.
- After adding TMB solution into the wells, the liquid in the wells gradually changes the color in blue. In this process the plate should be in dark. Remained TMB solution in the collecting container should not be returned into the original bottle of TMB solution to avoid contamination.
- Measurement of O.D. should be done within 30 minutes after addition of "7, Stop solution".

OPERATION MANUAL AND DOSAGES

1. Materials needed but not supplied.

Plate reader

Micropipette and tip

 Test tubes for dilution
 Deionized water
 Paper towel
 Incubator (37°C±1°C)

 Measuring cylinder and beaker
 Plate washer
 Collecting container
 (i.e. clean disposable test tube)
 Refrigerator

2. Preparation

- Preparation of wash buffer
 Dilute "8, Wash buffer conc." 40 fold with deionized water. The diluted one is used for the assay as a wash buffer. Adjust the required quantities if needed.
- Preparation of labeled antibody
 Dilute "2, Labeled antibody conc." 30 fold with "5, Solution for labeled antibody" using a prepared collecting container.
- Preparation of standard
 Add 0.5 mL of deionized water into the vial of "3, Standard" and completely dissolve it. Concentration of the standard is 3200 pmol/L. Prepare 7 test tubes for dilution of the standard and adding 230 µL of the EIA buffer into each tube.

Put 230 µL of 3200 pmol/L standard into the tube 1600 pmol/L (Tube-1) and gently mix it. Afterword, put 230 µL of the mixed liquid of tube-1 into the tube 800 pmol/L (Tube-2) and gently mix it. Dilute two fold standard solution in series to set up 7 points of diluted standard between 1600 pmol/L and 25 pmol/L.

Tube-1	1600	pmol/L
Tube-2	800	pmol/L
Tube-3	400	pmol/L
Tube-4	200	pmol/L
Tube-5	100	pmol/L
Tube-6	50	pmol/L
Tube-7	25	pmol/L

- Preparation of test samples
 Dilution ratio of Mouse EDTA-Plasma: 2 – 8 fold.
 Dilution ration of Mouse Urine: 200 – 400 fold.

3 MEASUREMENT PROCEDURE

- Add test sample blank
 Determine wells for test sample blank. Put 100µL each of "4, EIA buffer" into the wells.
- Add prepared test samples and standard
 Put 100 µL prepared test samples and 100 µL prepared standard into appropriate wells.
- Incubation with plate lid (1st reaction).
- Washing
 Wash the plate with the prepared wash buffer and remove all liquid.
- Add prepared labeled antibody
 Put 100 µL prepared labeled antibody into the wells.
- Incubation with plate lid (2nd reaction).
- Washing
 Wash the plate with the prepared wash buffer and remove all liquid completely.
- Add "6, Chromogen - TMB solution"
 Put 100 µL the TMB solution into the wells.
- Incubation in dark
- Add "7, Stop solution"
 Put 100 µL the Stop solution into the wells.
- Determination of optical density (O.D.)
 Remove any dirt or drop of water on the bottom of the plate and confirm there is no bubble on the surface of the liquid. Then, measure the both O.D. of standard and the test samples against a test sample blank.
 Measurement wavelength: 450 nm. In case of 2 wavelengths:
 Main wavelength is 450nm. Sub-wavelength is between 600 and 650 nm.

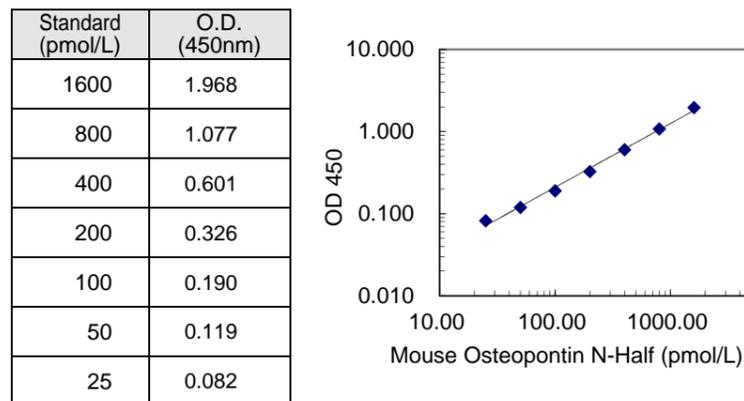
Table for measurement procedure

	Test samples	Standard	Test sample blank
Reagents	Test samples 100 µL	Diluted Standard 100 µL	EIA buffer 100 µL
1 st reaction	Incubation for 60 minutes at 37°C with plate lid.		
Washing	5 times (wash buffer more than 350 µL)		
Labeled antibody	100 µL	100 µL	100 µL
2 nd reaction	Incubation for 30 minutes at 2~8°C with plate lid.		
Washing	6 times (wash buffer more than 350 µL)		
TMB solution	100 µL	100 µL	100 µL
Chromogenic reaction	Incubation for 30 minutes at R.T. (shielded).		
Stop solution	100 µL	100 µL	100 µL
Measuring O.D.	450 nm / 600~650 nm		

CALCULATION OF TEST RESULT

- 1 Plot the concentration of the standard on the x-axis and its O.D. on the y-axis. Draw a standard curve by applying appropriate regression curve on each plot (i.e. quadratic regression of double logarithm conversion).
- 2 Read the concentration by applying the absorbance of the test samples on a standard curve.
- 3 Calculate the concentration of the test samples by multiplying dilution ratio of test samples on the value.

Example of standard curve and measured value


PERFORMANCE AND CHARACTERISTICS
1 Sensitivity

5 pmol/L

2 Measurement range

25 ~ 1600 pmol/L

3 Dilution linearity

Specimen	Titer (X)	Measurement Value (pmol/L)	Theoretical Value (pmol/L)	%
Mouse Urine	400	1450.99	1683.38	86.2
	800	747.25	802.90	93.1
	1600	372.27	379.80	98.0
	3200	182.17	179.72	101.4
	6400	93.77	87.90	106.7
Mouse Plasma (EDTA)	2	1139.44	1518.40	75.0
	4	698.81	807.02	86.6
	8	374.25	435.46	85.9
	16	192.97	222.97	86.5
	32	103.56	120.10	86.2
10%FCS added TIL Media I	2	252.10	566.73	44.5
	4	203.65	283.37	71.9
	8	124.17	141.68	87.6
	16	69.09	70.84	97.5
	32	37.37	35.42	105.5

4 Added recovery assay

Specimen	Theoretical Value (pmol/L)	Measurement Value (pmol/L)	%
Mouse Urine x400	1492.90	1379.85	92.4
	1117.90	1052.39	94.1
	930.40	894.52	96.1
	836.65	789.98	94.4
	789.78	753.14	95.4
Mouse EDTA – Plasma x 8	800	702.04	87.8
	400	363.57	90.9
	200	170.83	85.4
	100	86.67	86.7
	50	42.79	85.6
10%FCS added TIL Media I x4	800	726.07	90.8
	400	383.56	95.9
	200	173.01	86.5
	100	87.20	87.2
	50	42.79	85.6

5 Intra-assay

Measurement Value (pmol/L)	SD value (pmol/L)	CV value (%)	n
70.86	5.89	8.3	21
265.18	22.69	8.6	21
855.66	85.79	10.0	21

6 Inter-assay

Measurement Value (pmol/L)	SD value (pmol/L)	CV value (%)	n
74.92	6.38	8.5	16
202.19	15.25	7.5	16
757.81	69.29	9.1	16

PRECAUTION FOR INTENDED USE AND/OR HANDLING
1 Precaution for handling (Hazard prevention)

- (1) Treat the components carefully and wash hands after handling it.
- (2) "7, Stop solution" is a strong acid substance (1N Sulfuric acid). Therefore, it should be careful for the treatment and do not contact your skin and clothes with it. It also needs to pay attention to the disposal of it.

2 Precaution for intended use

- (1) "3, Standard" is lyophilized products. It should be careful to open this vial.
- (2) All reagents should be stored at 2 - 8°C.
- (3) Precipitation can be seen in "4, EIA buffer", "5, Solution for labeled antibody" and "8, Wash buffer conc.", however, it does not affect its performance.
- (4) Do not mix or replace the reagents with the reagents from a different lot or kit.
- (5) Do not use expired reagents.

3 Precaution for disposal

- (1) Dispose used materials after rinsing them with large quantity of water.

STORAGE AND THE TERM OF VALIDITY

Storage Condition: 2 - 8°C

The expiry date is specified on the outer box.

PACKAGE UNIT AND PRODUCT NUMBER

Package unit: 96 Well

Product number: 27259

CONTACT DETAILS

Immuno-Biological Laboratories Co., Ltd.
 1091-1 Naka, Fujioka-Shi, Gunma 375-0005
 TEL : 0274-22-2889
 FAX : 0274-23-6055