

Human Tenascin-C Large(FNIII-C) Assay Kit – IBL

96 Well

Please read carefully this instruction prior you use this assay kit.

INSTRUCTIONS FOR USE

This product is for research use only and is not intended for diagnostic use.

KIT COMPONENT

| | | |
|---|---|------------|
| 1 | Precoated plate: (Anti-Human Tenascin-C (19C4MS) Mouse IgG A.P.) | 96Well x 1 |
| 2 | Labeled antibody conc.: (30X) HRP conjugated Anti-Human Tenascin-C (4F10TT) Mouse IgG Fab'A.P.) | 0.4mL x 1 |
| 3 | Standard: (Purified Human Tenascin-C) | 0.5mL x 2 |
| 4 | EIA buffer | 30mL x 1 |
| 5 | Solution for labeled antibody | 12mL x 1 |
| 6 | Chromogen: | 15mL x 1 |
| 7 | Stop solution | 12mL x 1 |
| 8 | Wash buffer conc. | 50mL x 1 |

MEASURING SAMPLES

Human serum, heparin plasma and cell culture supernatant.

The plasma samples collected by EDTA, Citrate or NaF tend to give rather low data compare to assay by serum or heparin plasma.

PRINCIPLE

This kit is a solid phase sandwich ELISA (Enzyme-linked Immunosorbent Assay). As a primary antibody is coated on a plate, samples and standard are added into the wells for 1st reaction. After the reaction, HRP-conjugated secondary antibody is added into the wells for 2nd reaction. After washing away unbound the secondary antibody, Tetra Methyl Benzidine (TMB) is added to the wells and color develops.

OPERATING PRECATION

- Test samples should be measured soon after collection. For storage of samples, store them frozen and do not repeat freeze/thaw cycles. Thaw the test samples at a low temperature and mix them completely before measurement.
- Test samples should be diluted with "4, EIA buffer" contained in this kit.
- Duplicate measurement of test samples and standards is recommended.
- Standard curve should run for each assay.
- Use test samples in neutral pH range. The contaminations of organic solvent may affect the measurement.
- All reagents should be brought to room temperature (R.T.) and mixed completely and gently before use. After mixing them, make sure of no change in quality of the reagents.
- Use only "8, Wash buffer conc." contained in this kit for washing the precoated plate. Insufficient washing may lead to the failure in measurement.
- Wash the plate immediately after each reaction using by a plate washer with setting wait time zero second. The O.D. value tends to be lower if washing time is getting longer. If you use a multichannel pipette or a washing bottle due to no availability of any plate washer, filling wash buffer in each well and immediately turn the plate upside down and shake it off to completely remove the wash buffer. Repeat the number of times of wash defined in a table for measurement procedure described in section 3. It should be properly washed off as instructed in order to avoid any insufficient wash.
- Carefully tap the plate against a clean paper towel without contacting with inside of each well to completely remove the washing buffer after repeated the determined number of wash.
- "6, Chromogen - TMB solution" should be stored in the dark due to its sensitivity against light. It should be also avoided contact with metals. Required quantity should be prepared into a collecting container for each use.
- After adding TMB solution into the wells, the liquid in the wells gradually changes the color in blue. In this process the plate should be in dark. Remained TMB solution in the collecting container should not be returned into the original bottle of TMB solution to avoid contamination.
- Measurement of O.D. should be done within 30 minutes after addition of "7, Stop solution".

OPERATION MANUAL AND DOSAGES

1. Materials needed but not supplied.

| | |
|-------------------------|-----------------------------------|
| Plate reader | Micropipette and tip |
| Test tubes for dilution | Measuring cylinder and beaker |
| Deionized water | Plate washer |
| Paper towel | Collecting container |
| Refrigerator | (i.e. clean disposable test tube) |
| Incubator (37°C±1°C) | |

2. Preparation

(1) Preparation of wash buffer

Dilute "8, Wash buffer conc." 40 fold with deionized water. The diluted one is used for the assay as a wash buffer. Adjust the required quantities if needed.

(2) Preparation of labeled antibody

Dilute "2, Labeled antibody conc." 30 fold with "5, Solution for labeled antibody" using a prepared collecting container.

(3) Preparation of standard

Add 0.5 mL of deionized water into the vial of "3, Standard" and completely dissolve it. Concentration of the standard is 48 ng/mL. The standards enclosed in this kit can be frozen and stored after reconstitution. However the freeze-thaw shall not be repeated.

Prepare 7 test tubes for dilution of the standard and adding 230 µL of the EIA buffer into each tube.

Put 230 µL of 48 ng/mL standard into the tube 24 ng/mL (Tube-1) and gently mix it. Afterword, put 230 µL of the mixed liquid of tube-1 into the tube 12 ng/mL (Tube-2) and gently mix it. Dilute two fold standard solution in series to set up 7 points of diluted standard between 24 ng/mL and 0.38 ng/mL.

The standards enclosed in this kit can be frozen and stored after reconstitution. However the freeze-thaw shall not be repeated.

| | | |
|--------|------|-------|
| Tube-1 | 24 | ng/mL |
| Tube-2 | 12 | ng/mL |
| Tube-3 | 6 | ng/mL |
| Tube-4 | 3 | ng/mL |
| Tube-5 | 1.5 | ng/mL |
| Tube-6 | 0.75 | ng/mL |
| Tube-7 | 0.38 | ng/mL |

(4) Preparation of test samples

Dilute test samples with "4, EIA buffer" contained in this kit as follows.

Human serum and heparin plasma: more than 32 fold.*

Cell culture supernatant: more than 4 fold.

3 MEASUREMENT PROCEDURE

(1) Add test sample blank

Determine wells for test sample blank. Put 100µL each of "4, EIA buffer" into the wells.

(2) Add prepared test samples and standard

Put 100 µL prepared test samples and 100 µL prepared standard into appropriate wells.

(3) Incubation with plate lid (1st reaction).

(4) Washing

Wash the plate with the prepared wash buffer and remove all liquid.

(5) Add prepared labeled antibody

Put 100 µL prepared labeled antibody into the wells.

(6) Incubation with plate lid (2nd reaction).

(7) Washing

Wash the plate with the prepared wash buffer and remove all liquid completely.

(8) Add "6, Chromogen - TMB solution"

Put 100 µL the TMB solution into the wells.

(9) Incubation in dark

(10) Add "7, Stop solution"

Put 100 µL the Stop solution into the wells.

(11) Determination of optical density (O.D.)

Remove any dirt or drop of water on the bottom of the plate and confirm there is no bubble on the surface of the liquid. Then, measure the both O.D. of standard and the test samples against a test sample blank.

Measurement wavelength: 450 nm. In case of 2 wavelengths:

Main wavelength is 450nm. Sub-wavelength is between 600 and 650 nm.

Table for measurement procedure*


| | Test samples | Standard | Test sample blank |
|--------------------------|---|-------------------------------|----------------------|
| Reagents | Test samples 100 µL | Diluted Standard 100 µL | EIA buffer 100 µL |
| 1 st reaction | Incubation for 60 minutes at 37°C with plate lid. | | |
| Washing | 4 times (wash buffer more than 350 µL) (Refer to No. 8 and 9 described in OPERATING PRECATION.) | | |
| Labeled antibody | 100 µL | 100 µL | 100 µL |
| 2 nd reaction | Incubation for 30 minutes at 2~8°C with plate lid. | | |
| Washing | 5 times (wash buffer more than 350 µL) (Refer to No. 8 and 9 described in OPERATING PRECATION.) | | |
| TMB solution | 100 µL | 100 µL | 100 µL |
| Chromogenic reaction | Incubation for 30 minutes at R.T. (shielded). | | |
| Stop solution | 100 µL | 100 µL | 100 µL |
| Measuring O.D. | 450 nm / 600~650 nm | | |

CALCULATION OF TEST RESULT

- Plot the concentration of the standard on the x-axis and its O.D. on the y-axis. Draw a standard curve by applying appropriate regression curve on each plot (i.e. quadratic regression of double logarithm conversion).
- Read the concentration by applying the absorbance of the test samples on a standard curve.
- Calculate the concentration of the test samples by multiplying dilution ratio of test samples on the value.

Example of standard curve and measured value

| Standard (ng/mL) | O.D. (450nm) |
|------------------|--------------|
| 24 | 2.373 |
| 12 | 1.463 |
| 6 | 0.798 |
| 3 | 0.387 |
| 1.5 | 0.195 |
| 0.75 | 0.086 |
| 0.38 | 0.032 |

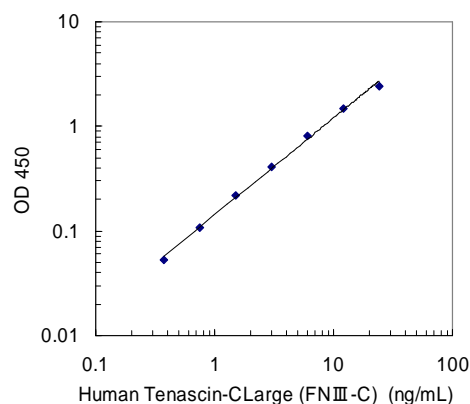

PERFORMANCE AND CHARACTERISTICS




1 Sensitivity

0.01 ng/mL (Calculated by NCCLS method using the standard.)

2 Measurement range

0.38 ~ 24 ng/mL

3 Dilution linearity*

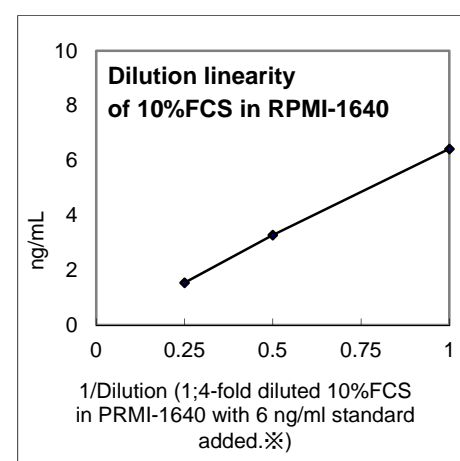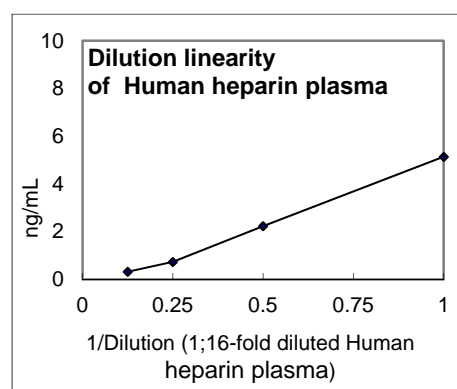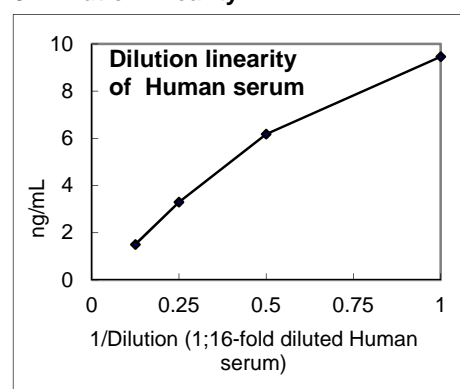

(※Samples with standard added are used.)

4 Added recovery assay*

| Specimen | Additive Amount (ng/mL) | Theoretical Value (ng/mL) | Measurement Value (ng/mL) | % |
|---------------------------|-------------------------|---------------------------|---------------------------|-------|
| 10%FCS in RPMI-1640 (x4) | 12.00 | 12.03 | 11.51 | 95.7 |
| | 6.00 | 6.03 | 5.45 | 90.4 |
| | 3.00 | 3.03 | 2.86 | 94.4 |
| Human Serum (x32) | 1.50 | 4.98 | 5.38 | 108.0 |
| | 0.75 | 4.23 | 4.80 | 113.5 |
| | 0.38 | 3.86 | 4.06 | 105.2 |
| Human heparin Plasma(x32) | 1.50 | 2.88 | 3.43 | 119.1 |
| | 0.75 | 2.13 | 2.42 | 113.6 |
| | 0.38 | 1.76 | 2.06 | 117.0 |

5 Intra-assay

| Measurement value (ng/ml) | SD(ng/ml) | CV (%) | n |
|---------------------------|-----------|--------|----|
| 13.54 | 0.52 | 3.8 | 22 |
| 3.22 | 0.14 | 4.3 | 22 |
| 0.91 | 0.06 | 6.6 | 22 |

6 Inter-assay*

| Measurement value (ng/ml) | SD (ng/ml) | CV (%) | n |
|---------------------------|------------|--------|---|
| 13.55 | 0.52 | 3.8 | 3 |
| 3.25 | 0.17 | 5.2 | 3 |
| 0.93 | 0.07 | 7.5 | 3 |

7 Specificity

Specifically detect Tenascin-C in human serum, heparin-plasma and cell culture supernatant.

PRECAUTION FOR INTENDED USE AND/OR HANDLING

1 Precaution for handling (Hazard prevention)

- Treat the components carefully and wash hands after handling it.
- "7, Stop solution" is a strong acid substance (1N Sulfuric acid). Therefore, it should be careful for the treatment and do not contact your skin and clothes with it. It also needs to pay attention to the disposal of it.

2 Precaution for intended use

- "3, Standard" is lyophilized products. It should be careful to open this vial.
- All reagents should be stored at 2 - 8°C.
- Precipitation can be seen in "4, EIA buffer", "5, Solution for labeled antibody" and "8, Wash buffer conc.", however, it does not affect its performance.
- Do not mix or replace the reagents with the reagents from a different lot or kit.
- Do not use expired reagents.

3 Precaution for disposal

- Dispose used materials after rinsing them with large quantity of water.

REFERENCE*

- Imanaka -Yoshida K et al. Tenascin-C is a useful marker for disease activity in myocarditis. *J Pathol.* 2002 Jul; 197(3):388-94.
- Tsunoda T et al. Involvement of large tenascin-C splice variants in breast cancer progression. *Am J Pathol.* 2003 Jun; 162 (6):1857-67.
- Hasegawa M et al. Tenascin-C concentration in synovial fluid correlates with radiographic progression of knee osteoarthritis. *J Rheumatol.* 2004 Oct; 31 (10):2021-6.
- Imanaka-Yoshida K et al. Interaction between cell and extracellular matrix in heart disease: multiple roles of tenascin-C in tissue remodeling. *Histol Histopathol.* 2004 Apr; 19 (2):517-25.
- Hasegawa M et al. Tenascin-C levels in pseudosynovial fluid of loose hip prostheses. *Scand J Rheumatol.* 2005 Nov-Dec; 34 (6):464-8.
- Morimoto S et al. Diagnostic utility of tenascin-C for evaluation of the activity of human acute myocarditis. *J Pathol.* 2005 Mar; 205 (4):460-7.
- Sato A et al. Serum tenascin-C might be a novel predictor of left ventricular remodeling and prognosis after acute myocardial infarction. *J Am Coll Cardiol.* 2006 Jun 6; 47 (11):2319-25.
- Tanaka H et al. Circulating level of large splice variants of tenascin-C is a marker of piecemeal necrosis activity in patients with chronic hepatitis C. *Liver Int.* 2006 Apr; 26 (3):311-8.
- Fujimoto N et al. Incremental prognostic values of serum tenascin-C levels with blood B-type natriuretic peptide testing at discharge in patients with dilated cardiomyopathy and decompensated heart failure. *J Card Fail.* 2009 Dec;15(10):898-905.

STORAGE AND THE TERM OF VALIDITY

Storage Condition: 2 - 8°C

The expiry date is specified on the outer box.

PACKAGE UNIT AND PRODUCT NUMBER

Package unit: 96 Well

Product number: 27751

CONTACT DETAILS*

Immuno-Biological Laboratories Co., Ltd.

1091-1 Naka, Fujioka-Shi, Gunma 375-0005, Japan

URL: <https://www.ibl-japan.co.jp/en/>

E-mail: do-ibl@ibl-japan.co.jp